SIEMENS

MammoReport^{Plus}

SP

System Manual

Wiring Diagrams

© Siemens AG 2005
The reproduction, transmission or use of this document or its contents is not permitted without express written authority. Offenders will be liable for damages. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

Register 6
Print No.: SPB7-420.844.20.02.02

English
Doc. Gen. Date: 06.05

Chapter	Page	Revision
All	All	01

Document revision level

The document corresponds to the version/revision level effective at the time of system delivery. Revisions to hardcopy documentation are not automatically distributed.

Please contact your local Siemens office to order current revision levels.

Disclaimer

The installation and service of equipment described herein is to be performed by qualified personnel who are employed by Siemens or one of its affiliates or who are otherwise authorized by Siemens or one of its affiliates to provide such services.

Assemblers and other persons who are not employed by or otherwise directly affiliated with or authorized by Siemens or one of its affiliates are directed to contact one of the local offices of Siemens or one of its affiliates before attempting installation or service procedures.

Copyright notice

The DICOM functionalities in the MammoReportPlus system are based on the libraries from Merge Technologies Inc.

Celsius R610 is a trademark of Fujitsu Siemens Computers.

Windows XP Professional is a trademark of Microsoft Corporation.
SIMOMED SMM 21201P, DSB 2103-D-5MP and syngo are trademarks of Siemens AG.

Softcopy reading software by MeVis BreastCare,
copyright © 2001 - 2005 by MeVis BreastCare.

Contents

Page

1 System overview 1-1

General 1-1
MammoReportPlus system overview 1-1

2 Cables 2-1

Cable connections 2-1

3 Connectors 3-1

Workstation connectors (CRT monitors) 3-1
Workstation connectors (Siemens/Barco TFT monitors) 3-2

4 Changes to previous version 4-1

Contents

Page

General

This document describes the main functions of the MammoReport^{Plus} system and the electrical connections between the parts.

MammoReport^{Plus} system overview

An overview of the MammoReport^{Plus} system is provided below.

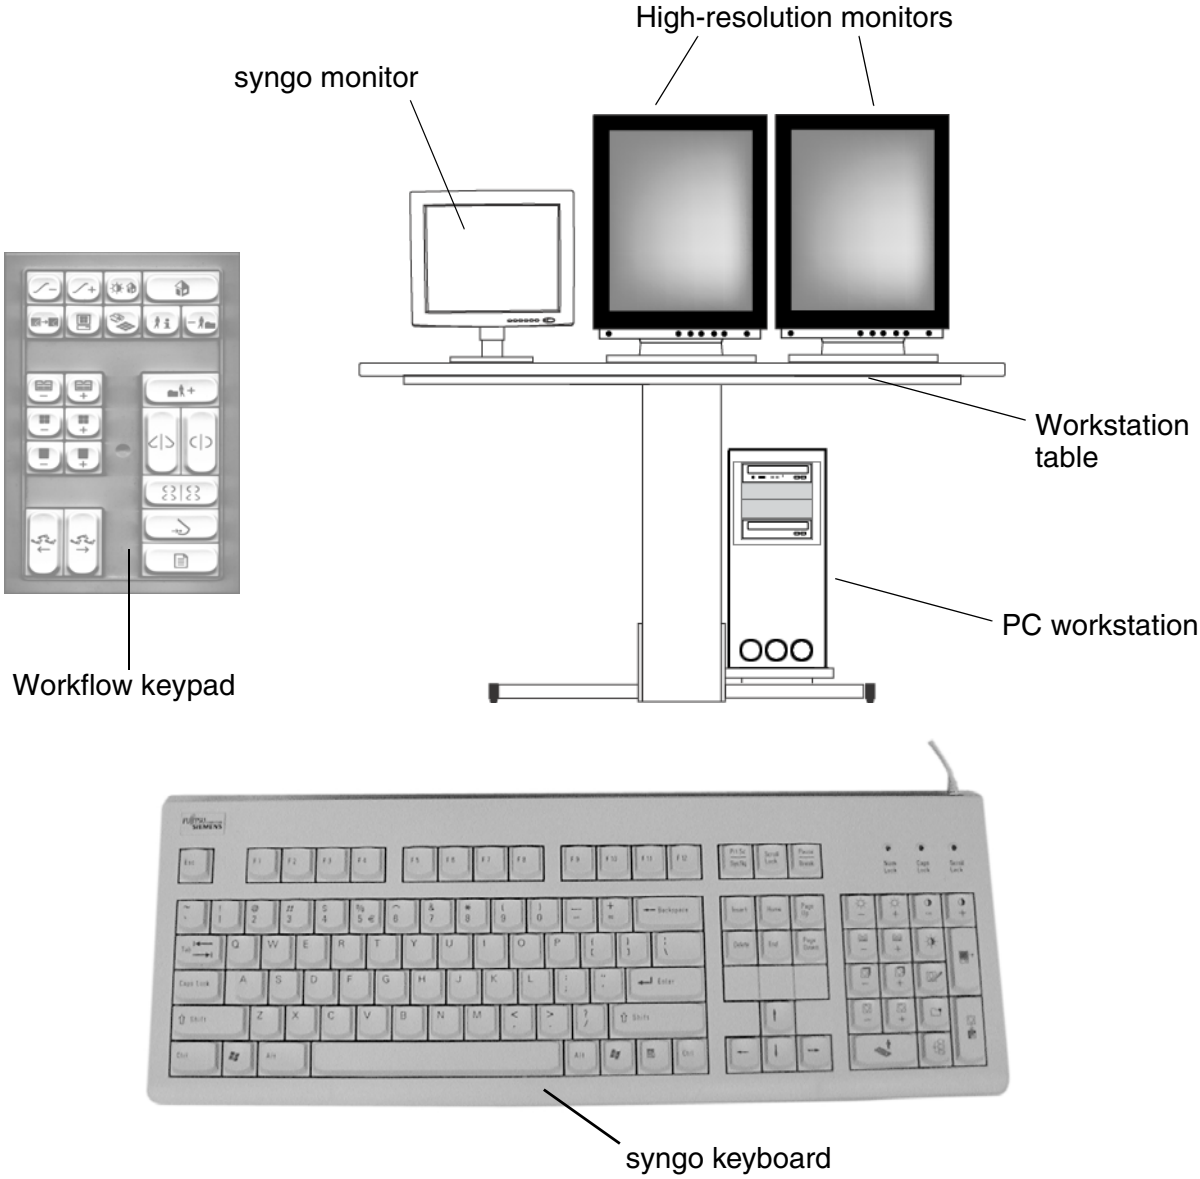

The MammoReport^{Plus} system's major parts are:

- 2 Displays
  - Either high-resolution monitors - SIMOMED SMM21201P (CRT)
  - or TFT monitors (DSB 2103-D-5MP) or (Barco MFGD 5621 HD)
- FSC Celsius R610 workstation
- Workflow keypad
- MammoReport^{Plus} software
- syngo keyboard
- syngo monitor
- Windows XP professional compatible printer, provided by the customer

Additional options to the MammoReport^{Plus} system are:

- One additional 147 GB hard disk

NOTE	**For current system options, see price book.**

Cable connections

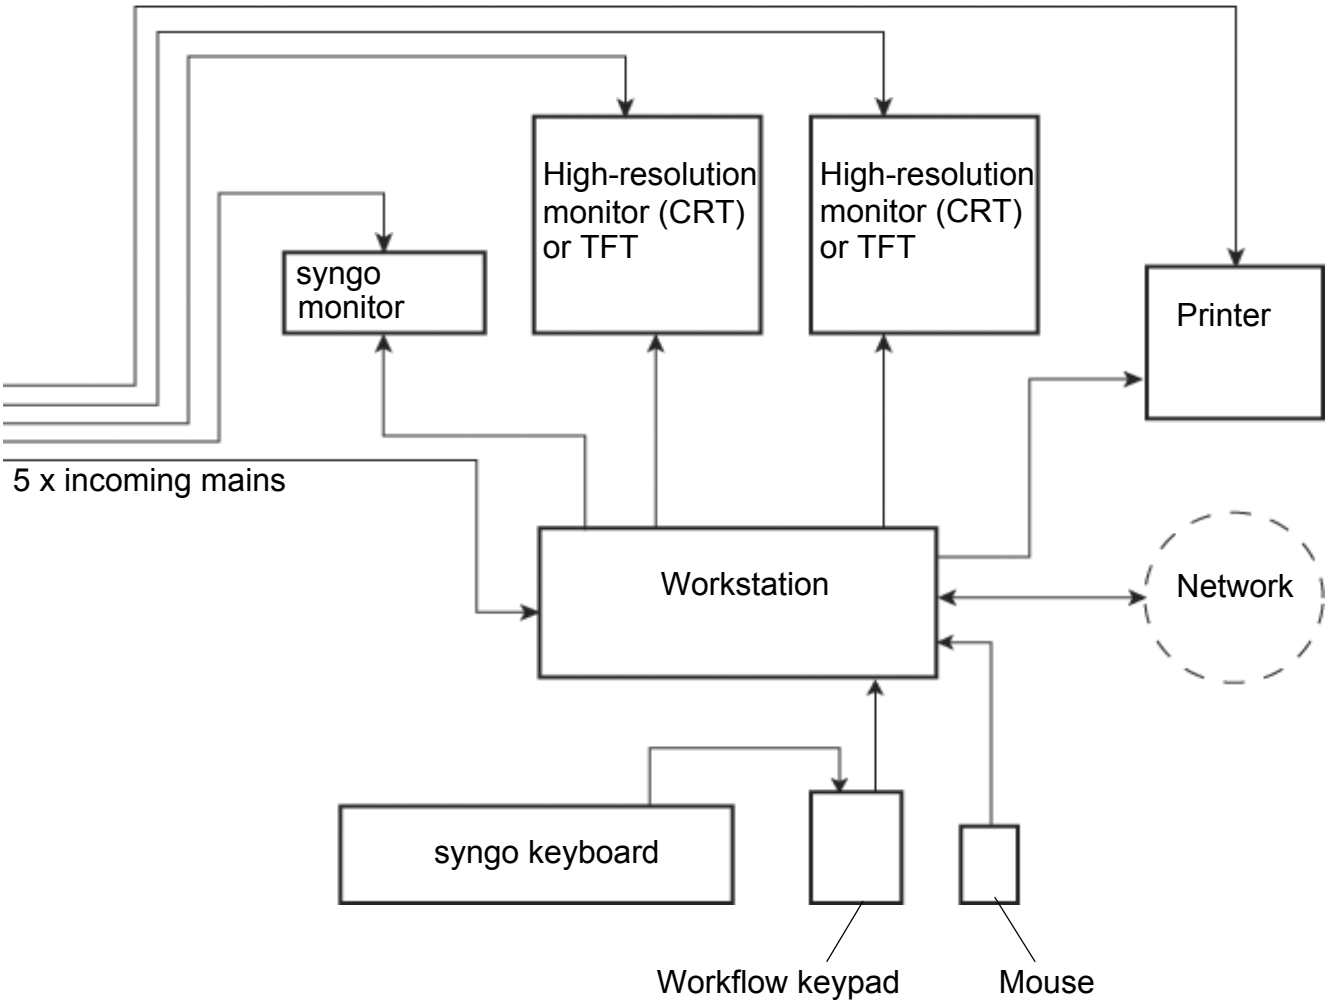

Fig. 1 Cable connections

NOTE	**The MammoReport^{Plus} system can be connected to line voltage 100-240 V.**

This page intentionally left blank.

Workstation connectors (CRT monitors)

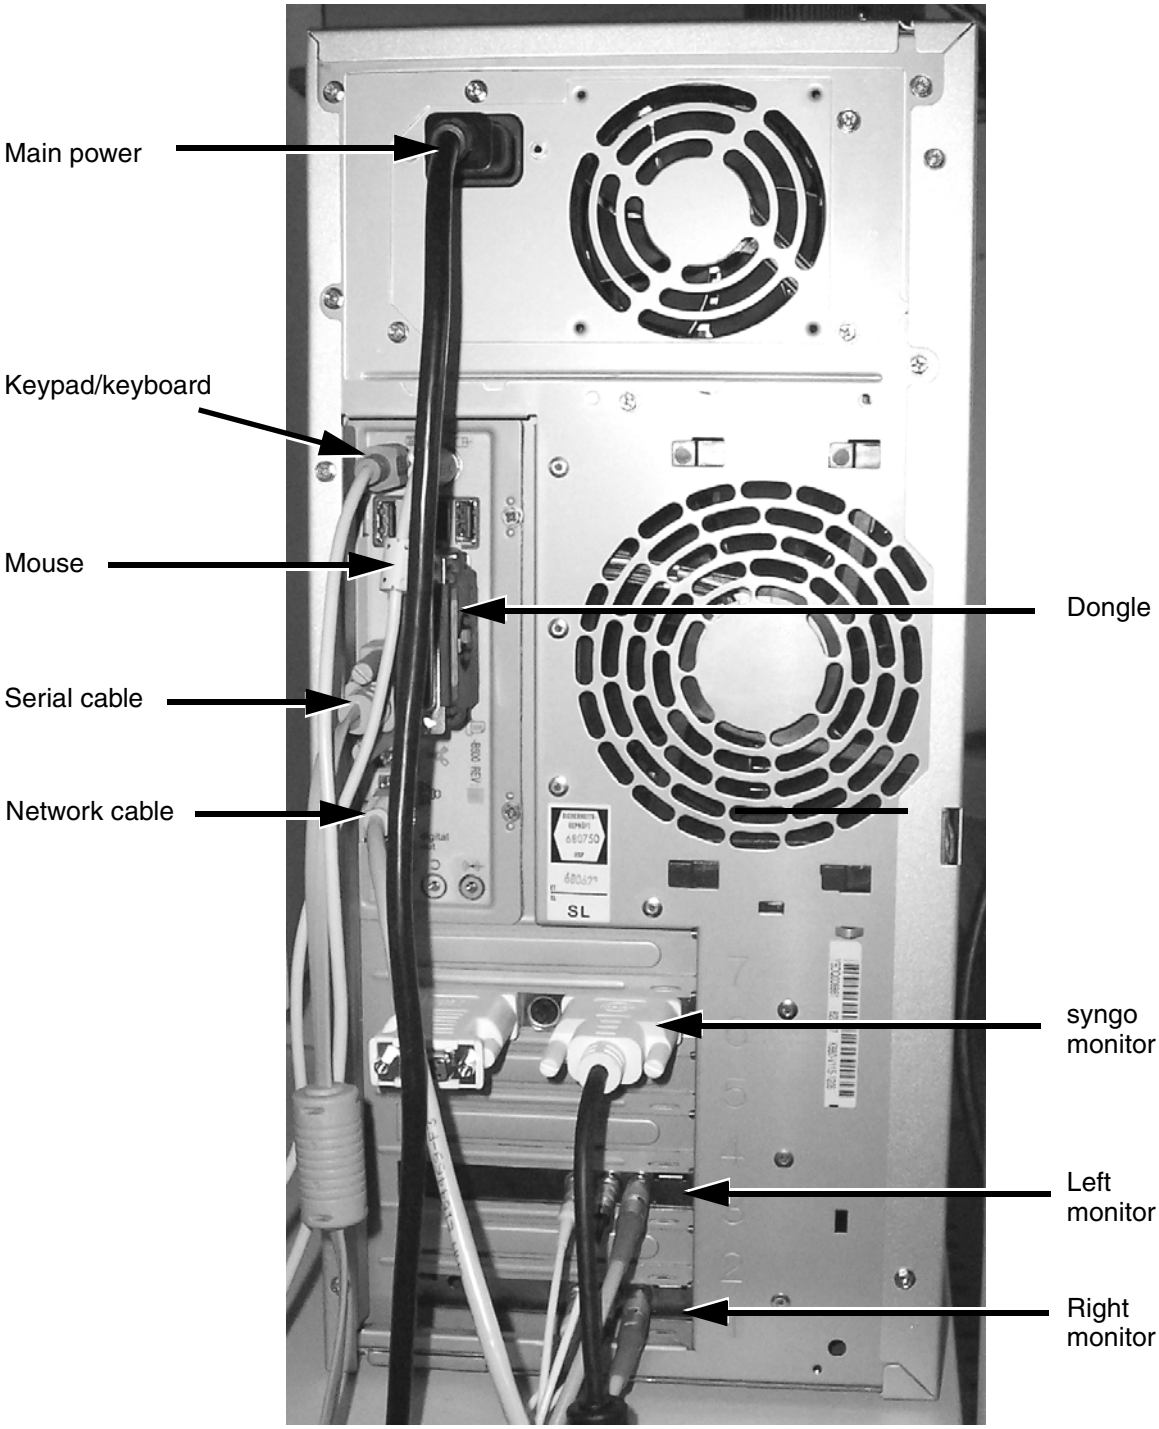

Fig. 1 Connectors FSC Celsius R610

Workstation connectors (Siemens/Barco TFT monitors)

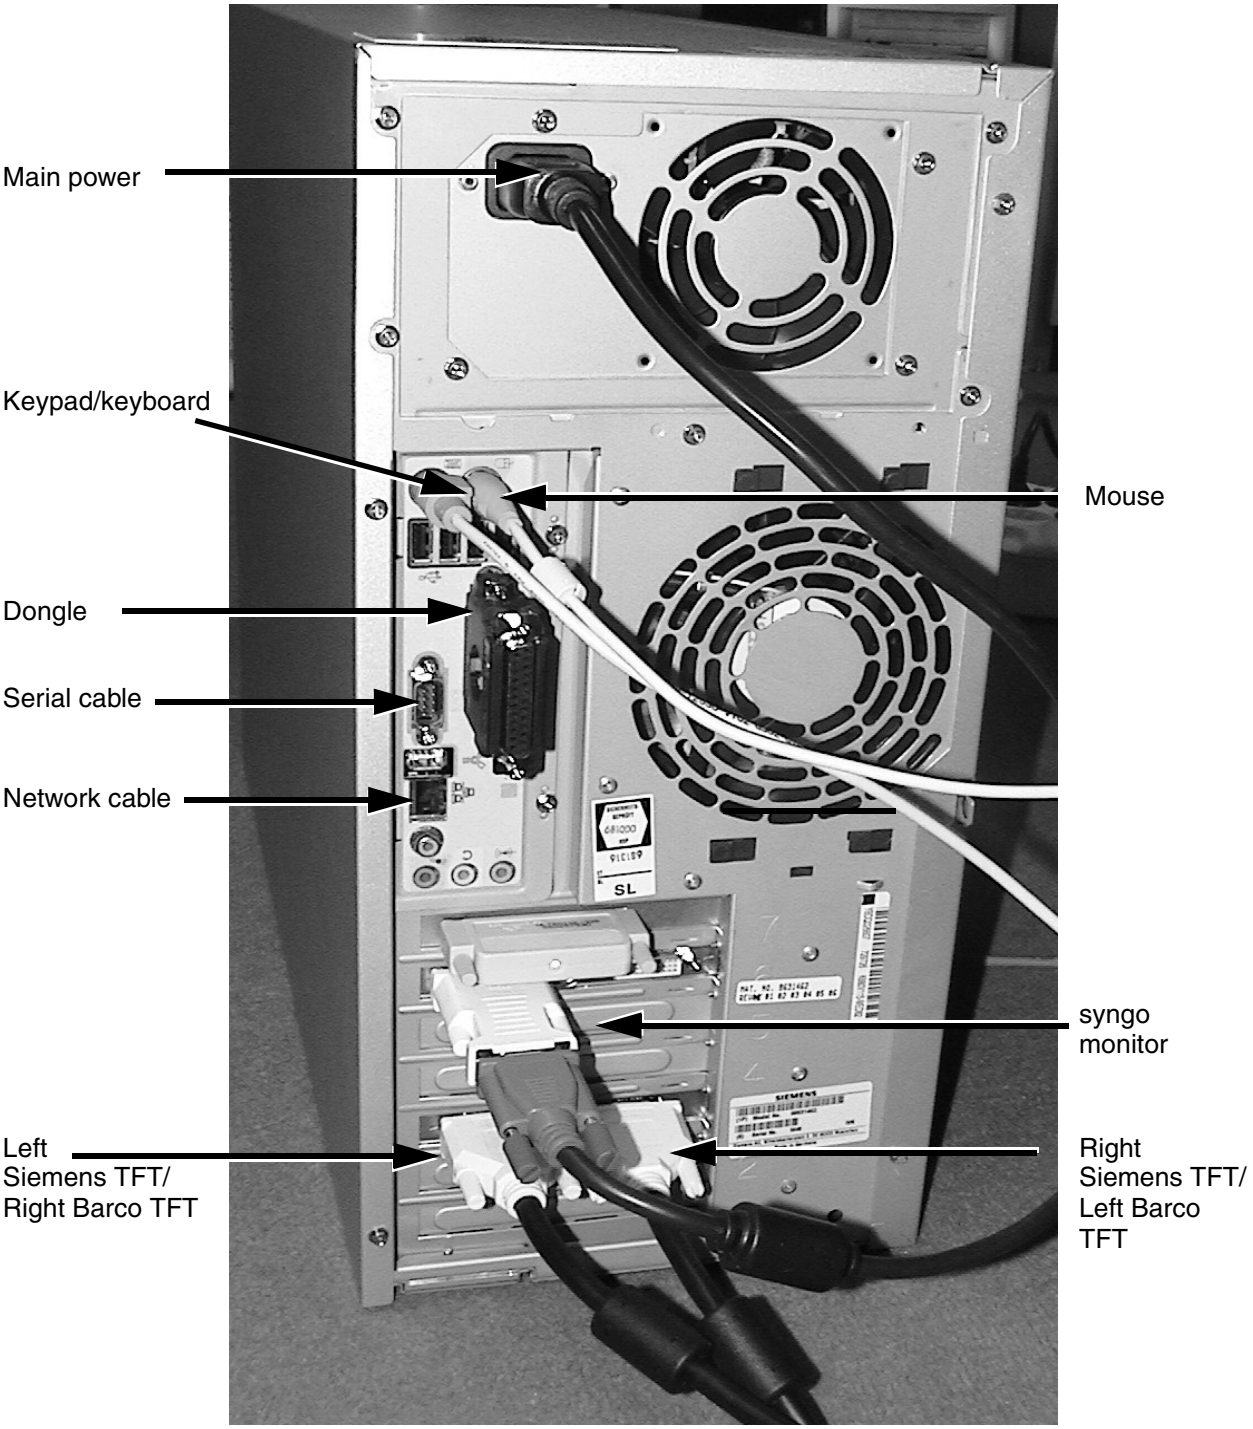

Fig. 2 Connectors FSC Celsius R610

1

Chapter	Page	Change
	1-2	add Barco TFT

This page intentionally left blank.